

Thank you for purchasing an Agilent instrument. To get you started and to assure a successful and timely installation, please refer to this specification or set of requirements.

Correct site preparation is the key first step in ensuring that your instruments and software systems operate reliably over an extended lifetime. This document is an **information guide AND checklist** prepared for you that outlines the supplies, consumables, space and utility requirements for your equipment for your site.

For additional information about our solutions, please visit our web site at http://www.chem.agilent.com/en-us/Pages/HomePage.aspx

Make sure your site meets the following prior to the installation date using the checklist below. For details, see specific sections within

Customer Responsibilities:

this docu	ment, including:
	The necessary laboratory or bench space is available.
	The environmental conditions for the lab as well as laboratory gases, tubing.
	The power requirements related to the product (e.g. number & location of electrical outlets).
	The required operating supplies necessary for the product and installation.
	Please consult Other/Special Requirements section below for other product-specific information.
	For more details, please consult the product-specific Site Prep manual (delete this line if a Site Prep Guide does not exist).
	If Agilent is delivering installation and familiarization services, users of the instrument should be present throughout these services; otherwise, they will miss important operational, maintenance and safety information.
	When using hydrogen (H2) as the carrier gas or fuel gas, be aware that hydrogen gas can flow into the GC oven and create an explosion hazard. Therefore, be sure that the supply is turned off until all connections are made and ensure that the inlet and detector column fittings are either connected to a column or capped at all times when hydrogen gas is supplied to the instrument. Hydrogen is flammable. Leaks, when confined in an enclosed space, may create a fire or explosion hazard. In any application using hydrogen, leak test all connections, lines, and valves before operating the instrument. Always turn off the hydrogen supply at its source before working on the instrument. Please refer to the Hydrogen Safety Guide which is shipped with the Instrument.

Issued: 03 February 2019 Copyright © 2019 Agilent

Rev: B.01.09 Page 1 of 14



Important Customer Information

- If you have questions or problems in providing anything described as a Customer Responsibilities above, please
 contact your local Agilent or partner support/service organization for assistance prior to delivery. In addition,
 Agilent and/or its partners reserve the right to reschedule the installation dependent upon the readiness of your
 laboratory.
- 2. Should your site not be ready for whatever reasons, please contact Agilent as soon as possible to re-arrange any services that have been purchased.
- 3. Other optional services such as additional training, operational qualification (OQ) and consultation for user-specific applications may also be provided at the time of installation when ordered with the system, but should be contracted separately.
- 4. Please refer to the other Products (ie; GC, ALS, CTC, etc) for site preparation requirements.

Issued: 03 February 2019 Copyright © 2019 Agilent

Rev: B.01.09 Page 2 of 14



7000 and 7010 Tandem Quad System





Dimensions and Weight

Identify the laboratory bench space before your system arrives based on the table below.


Pay special attention to the total height and total weight requirements for all system components you have ordered and avoid bench space with overhanging shelves. Also pay special attention to the total weight of the modules you have ordered to ensure your laboratory bench can support this weight.

Issued: 03 February 2019 Copyright © 2019 Agilent Page 3 of 14

B.01.09 Rev:



Typical GC/MS System - 8890 GC, 7000 or 7010 MSD, with computer and printer.

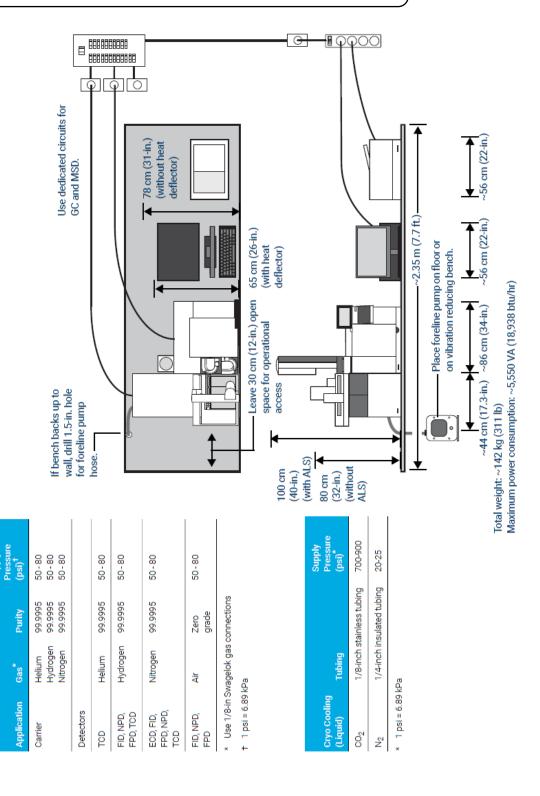

Issued: 03 February 2019 Copyright © 2019 Agilent Rev: B.01.09 Page 4 of 14



Special Notes:

- 1. This does not include the automated sampling devices which could be used on the system.
- 2. Please note: the length of the vacuum hose is 130 cm or about 4.24 feet from the high vacuum pump to the foreline pump, while the length of the foreline pump power cord is 2 M or about 6.6 feet.
- 3. A table must be large enough to support the mainframe and the size of the base plus additional accessories.
- 4. The dimensions and weight of the instrument needs to be placed on a laboratory bench that is at least 101 cm (40 in) deep. The instrument requires a space of at least 40.0 cm (16 in) on both sides, and approximately 30 cm (~ 12 in) at the rear for the circulation of air, vacuum pump hose, and room for electrical connections.
- 5. If the bench is to support a complete Agilent 7000 or 7010 GC/MS system make sure that the bench is designed to carry the total weight of all the components.

DESCRIPTION	Weight		Height		Depth		Width	
DESCRIFTION	kg	lbs	cm	in	cm	in	cm	in
Tandem Quad EI or HES (on the bench)	59	130	47	18.5	86	34	35	14
Tandem Quad EI/CI or HES/CI (on the bench)	63.5	140	47	18.5	86	34	35	14
Tandem Qud shipping container	90	198	75	29.5	69	27.5	113	44.5
RV5 – Foreline Pump - Wet	25	55	26.7	10.5	43.0	16.9	15.8	6.22
IDP-10 – Foreline Pump - Dry	24.7	54.5	29.7	11.7	42.0	16.5	26.0	10.2
IDP-10 – Foreline Pump – Dry shipping container	28.1	62	45.7	18	40.6	16	70	24
Workstation PC system (monitor, CPU, printer)	50	112	54	21.3	54	21.3	54	21.3
System shipping container (varies)	175	385	91	36	96	38	130	51

Issued: 03 February 2019 Copyright © 2019 Agilent Page 5 of 14

B.01.09 Rev:





Environmental Conditions

Operating your instrument within the recommended temperature ranges insures optimum instrument performance and lifetime.

Special Notes:

- 1. Performance can be affected by sources of heat & cold e.g. direct sunlight, heating/cooling from air conditioning outlets, drafts and/or vibrations.
- 2. The site's ambient temperature conditions must be stable for optimum performance of the system's modules as specified in the "Environmental Specifications" section of the Site Preparation Manual. Temperature changes should not exceed 3°C from its intended set-point to achieve best possible baseline stability. Higher variations will result in higher signal drift and wander of the baseline.
- 3. The bench or supporting surface must be vibration free.
- 4. The following table may help you calculate the additional BTUs of heat dissipation from this new equipment. Maximums represent the heat given off when heated zones are set for maximum temperatures.

Instrument Description	Operating temp range °C	Operating humidity range (%)	Heat Dissipation (BTU)
Tandem Quad GC GC/MS	15 to 35 °C	20% - 80%	6200 BTU / hour
			including GC/MS interface



Exhaust Venting Requirements

The foreline pump exhaust is recommended to be vented outside of the laboratory environment. Exhaust vent system should not be part of an environmental control system that recirculates air inside of a building. Exhaust venting requirements need to comply with all local environmental and safety codes. If the exhaust is non-toxic then an oil mist filter should be used on the foreline pump exhaust.

- 1. A 6-meter (20ft.) length (cut to length for the location of the instrument) of 1/2 in id PVC/vinyl tubing is recommended for venting the foreline pump exhaust. This is sufficient for two three-meter (10-foot lengths).
- 2. The foreline pump exhaust should not be shared with exhaust tubing from another instrument. Separate $\frac{1}{2}$ inch hose barbs are required to connect the tubing to the exhaust vent.

Issued: 03 February 2019 Copyright © 2019 Agilent

Rev: B.01.09 Page 6 of 14





Power Consumption

Special Notes:

If a computer system is supplied with your instrument, be sure to account for all electrical outlets.

Instrument Description	Line Voltage & Frequency (V, Hz)	Maximum Power Consumption (VA)			
Tandem Quad GC GC/MS	120VAC (-10% / + 5%) 50/60 Hz ± 5%	1100VA (1200VA for foreline pump only)			
	200-240VAC (-10% / + 5%) 50/60 Hz ± 5%	1100VA (1200VA for foreline pump only)			
	120VAC (-10% / + 5%),	1000VA			
Workstation PC system (dual monitor, CPU,	50/60 Hz ± 5%				
optional printer)	200-240VAC (-10% / + 5%),	1000VA			
	50/60 Hz ± 5%				

Part Number	Line Voltage Power Cords for the GC QTOF (C19)	
8120-6360	Power Cord, Taiwan/S America, C19, 20A	
8120-6903	Power Cord, Japan, C19, 20 amp	
8120-8619	Power Cord, Australia, C19, 16 amp	
8120-8620	Power Cord, GB/HK/SG/MY, C19, 13 amp	
8120-8622	Power Cord, Swiss/DK, C19, 16 amp	
8121-0070	Power Cord, China, C19, 15 amp, Fast	
8121-0161	Power Cord, Israel, C19, 16 Amp	
8121-0675	Power Cord, Argentina, C19, 16 amp	
8121-0710	Power Cord,India/S.Africa, C19, 15 Amp	
8121-1222	Power Cord, Europe+S Korea, C19, 15A, 250V	
8121-1301	Power Cord, Thai 220V, 15 A, 1.8M, C19	
8121-1787	Power Cord, Brazil, C19, 250V Max	
8121-0075	Power Cord, US 240V, C19, 15 amp	

Issued: 03 February 2019 Copyright © 2019 Agilent Page 7 of 14

Rev: B.01.09



Part Number	Line Voltage Power Cords for the CPU/Monitor/Printer (C13)
8120-0674	Power cord - Thailand and Philippines
8120-1369	Power Cord, Australia/NZ, C13, 10 amp
8120-2104	Power Cord, Switzerland, C13, 10 amp
8120-3997	Power Cord, DK/Greenland, C13, 10 amp
8120-4211	Power Cord, India/S Africa, C13, 10 amp
8120-5182	Power Cord, Israel, C13, 10 amp
8120-6869	Power Cord, Argentina, C13 250V 10A RA/3
8120-6978	Power Cord, Chile, C13, 10 amp
8120-8705	Power Cord, GB/HK/SG/MY, C13, 10 amp
8121-0723	Power Cord, China, C13, 10 A, 250V
8121-1226	Power Cord,Europe+S Korea C13, 10A, 250V
8121-1635	Power cord - Taiwan
8121-1638	Power cord - Cambodia
8121-1809	Power Cord, Brazil, C13, 250V Max
8120-1378	Power Cord C13 125V 10A 5-15P 498G US
8120-4753	Power Cord, Japan, C13, 125V

Part Number	Line Voltage Power Cords for the Switch (C7)	
8120-6313	Power Cord, US, C7, 125V,2.5A, 1-15P Plg	
8120-8336	Power Cord, Japan, 2- wire, C7,125V,7A	
8120-8337	Power Cord, Australia, 2 wire	
8120-8340	Power Cord, Europlug, C7, 250V Max, 2.5A	
8120-8346	Power Cord, China, 2 wire	
8120-8420	Power Cord Korea	
8120-8421	Power Cord India / South Afri	
8120-8452	Power Cord South America	
8120-8719	Power Cord, UK	
8120-8367	Power-Cord OPT-950 2-COND 1.8-M-LG	

Issued: 03 February 2019 Copyright © 2019 Agilent Page 8 of 14

Rev: B.01.09





Required Operating Supplies by Customer

Special Notes:

For information on Agilent consumables, accessories and laboratory operating supplies, please visit http://www.chem.agilent.com/en-US/Products/consumables/Pages/default.aspx

Item Description, (including dimensions etc)	Vendor/Part Number (if applicable)	Recommended Quantity
Analytical Table	www.onepointesolutions.com	1
H-31" D-40" W-96"	www.ChemTops.com	
Noise Chamber for foreline pumps, coasters		
Computer Table	www.onepointesolutions.com	1
(if table is same depth then they can be placed next to each other)		
H-31" D-40" W-36"	www.ChemTops.com	
Monitor support rack and Keyboard rack, coasters		
Table is just large enough to hold GC QTOF and GC.	Mass Spec Bench, G3215A	1



Other/Special Requirements

Gases are supplied by tanks, internal distribution system, or gas generators. Tank supplies require two staged, pressure regulation.

To connect tubing to the supply, it must have one 1/8-inch Swagelok female connector for each gas. Make sure that your regulator has the appropriate sized adapter to end with a 1/8-inch Swagelok female connector. (The URL of Swagelok's web site is http://www.swagelock.com to help assist is finding connectors.) It is recommend two (2) step regulators be used with 1/8" size outlets.

Issued: 03 February 2019 Copyright © 2019 Agilent Page 9 of 14

B.01.09 Rev:



Tandem Quad Gas Flow Limitations

Feature	7000/7010 Series
High Vacuum Pump Type	Split-Flow Turbo
Carrier Gas Optimal gas flow ml/min (a)	1.0 – 1.5
Carrier Gas Max recommended gas flow, ml/min	2.0
Carrier Gas Max gas flow, ml/min (b)	2.4
Collision Cell Gas Flow Rate (Nitrogen/Helium – via CC EPC module)	5 ml/min
Reagent Gas Flow (EI/CI or HES/CI – CI application – 25 PSI upper limit, Methane) (c)	1.0 – 2.0
Max column id	0.32mm (30m)

- a Total gas flow into the MS: column flow plus reagent gas flow (if applicable)
- b Expect degradation of spectral performance and sensitivity
- c Upper gas limits will vary depending upon the gas type being used
- 1. Purity specification given is the minimum acceptable purity. Major contaminates can be water, oxygen, or air.
- 2. Pre-cleaned 1/8" copper tubing and 1/8-in Swagelok® fittings are supplied as part of the ship kit to connect the collision cell gas to the collision cell inlet fitting.
- 3. Never use liquid thread sealer to connect fittings.

Tandem Quad Series Carrier and Reagent Gases

Carrier and reagent gas requirements	Typical pressure range (psi)	Typical flow (ml/min)
Helium (required)	50 to 80	20 to 100
		(column and split flow)
Hydrogen	50 to 80	20 to 50
		(column and spilet flow)
Methane Reagent Gas	15 to 25	1 to 2
(required for CI operation)		
Isobutane reagent gas (optional)	15 to 25	1 to 2
Ammonia reagent gas (optional)	5 to 8	1 to 2
Carbon dioxide reagent gas (optional)	15 to 20	1 to 2

Rev: B.01.09 Page 10 of 14



Tandem Quad Series CC Gases

Carrier and reagent gas requirements	Typical pressure range (psi)	Typical flow (ml/min)
7000 Helium (required) via GC EPC CC Module (a)	50 to 80	2.25
7000 Nitrogen (required) via GC EPC CC Module (a)	50 to 80	1.5
7010 Helium (required) via GC EPC CC Module	50 to 80	4.0
7010 Nitrogen (required) via GC EPC CC Module	50 to 80	1.0

a Optimal performance for 7010 is listed below, but if one uses the 7000 values then no changes with the collision cell energies will be required. Typically, the 7010 optimal values are 3-6 volts higher than the 7000 values.



Gas Selection

Agilent recommends that carrier and detector gases be 99.9995% pure. Air needs to be zero grade or better. Agilent also recommends using traps to remove hydrocarbons, water, and oxygen.

Tandem Quad Carrier and Reagent Gases Purity

Carrier and reagent gas requirements	Purity	Note
Helium (Carrier)	99.9995%	hydrocarbon free
Hydrogen (Carrier)	99.9995%	SFC Grade
Nitrogen (Collision Cell via GC EPC)	99.999%	Research or SFC grade
Methane Reagent Gas	99.999%	Research or SFC grade
(required for CI opeation)		
Isobutane Reagent Gas (optional)	99.99%	Instrument grade
Ammonia Reagent Gas (optional)	99.9995%	Research or SFC grade
Carbon Dioxide Reagent Gas (optinal)	99.995%	SFC Grade

It is recommend two (2) step regulators be used with 1/8" size outlets.

- 1. Purity specification given is the minimum acceptable purity. Major contaminates can be water, oxygen, or air.
- 2. Pre-cleaned 1/8" copper tubing and 1/8-inch Swagelock ® fittings are supplies as part of the ship kit.
- 3. Pre-cleaned 1/8" stainless-steel tubing and 1/8-inch Swagelock ® fittings are supplies as part of the ship kit; CI instruments
- 4. Never use liquid thread sealer to connect fittings.

Issued: 03 February 2019 Copyright © 2019 Agilent

Rev: B.01.09 Page 11 of 14





Remote Diagnostics

Easy access to diagnostic information and to the system operator helps our service engineers diagnose problems or share information. We recommend these features to help support your new system:

- 1. A LAN connection for the Data Acquisition and Data Analysis PC is recommended to provide remote diagnostics capability for the Tandem Quad Series GC/MS System.
- 2. A phone line close to the instrument is strongly recommended for communication with the system operator.



Other considerations

Basic Tools

Your GC-QTOF comes with a few basic tools and consumables depending on the specific inlet and detector that you ordered. Here is a general list which one will get with the instruments or should have on-hand.

Tool or consumable	Used for
Inlet wrench	Replacing inlet septa and liners.
T10 and T20 Torx wrenches	Remove tray. Remove covers to access EPC modules, traps, and possible leaks.
Column cutter	Column installation.
1/8-inch Tee, Swagelok, brass	Connect gas supplies
1/8-inch nuts & ferrules, Swagelok, brass	Connect gas supplies
1.5 mm and 2.0 mm hex driver	Source maintenance (disassembly)
Tool bag	Used to hold GC and MS tools
Q-Tips	Used to clean source parts
Cloths	Used to keep surfaces clean and parts clean
Gloves	Used to reduce contamination on parts GC and MS

MS Maintenance supplies	
Description	Part number
Abrasive paper, 30 μm	5061-5896
Alumina powder	393706201
Cloths, clean (package of 15)	05980-60051
Cloths, cleaning (package of 300	9310-4828
Cotton swabs (package of 100)	5080-5400

Issued: 03 February 2019 Copyright © 2019 Agilent

Rev: B.01.09 Page 12 of 14



0030 0029 0289 3308 3507 3508
3308 3507 3508
3308 3507 3508
3507 3508
3507 3508
3507 3508
3508
3508
3506
3323
3514
3512
2-60001
-5348
-5347
-0585
65201
1-60571
8510
0-60045
2

Issued: 03 February 2019 Copyright © 2019 Agilent
Rev: B.01.09 Page 13 of 14



Important Customer Web Links

For additional information about our solutions, please visit our web site

http://www.chem.agilent.com/

Need to get information on your product? Literature Library - Need to know more? Customer Education - Need technical support, FAQs? - Need supplies? -

http://www.agilent.com/chem/library http://www.agilent.com/chem/education http://www.agilent.com/chem/techsupp http://www.agilent.com/chem/supplies

Issued: 03 February 2019 Copyright © 2019 Agilent

Rev: B.01.09 Page 14 of 14