

## Effective HPLC Determination of Fentanyl using ELSD

Stephen Bullock  
Polymer Laboratories, now a part of Varian, Inc.

### Introduction

Fentanyl was first synthesized in Belgium in the late 1950s. To date, over 12 different analogs of fentanyl have been produced and identified in the US drug traffic. There is, therefore, a requirement to screen urine samples, both from human and animal sources, and to detect and quantify fentanyl present in very low concentrations.

In this experiment, an isocratic HPLC method was used to analyze samples of fentanyl prepared at fixed concentrations over the range 0.5 µg/mL up to 200 mg/mL. The Varian evaporative light scattering (ELS) detector was employed because of its superior performance; the detection method is independent of the optical properties of the compound under consideration.

### Instrumentation

Column: Silica C18 5 µm, 50 x 2.1 mm  
Detector: Varian ELSD (neb=40 °C, evap=70 °C, gas=1.2 SLM)

### Materials and Reagents

Eluent: 60 % 0.25 M Ammonium acetate in water, 40 % Acetonitrile

### Sample Preparation


Concentration: 0.5–200 µg Fentanyl/mL

### Conditions

Flow Rate: 0.25 mL/min  
Injection Volume: 10 µL


### Results and Discussion

Figure 1 shows typical chromatograms obtained for two concentrations of fentanyl within the range 0.5–200 µg/mL.

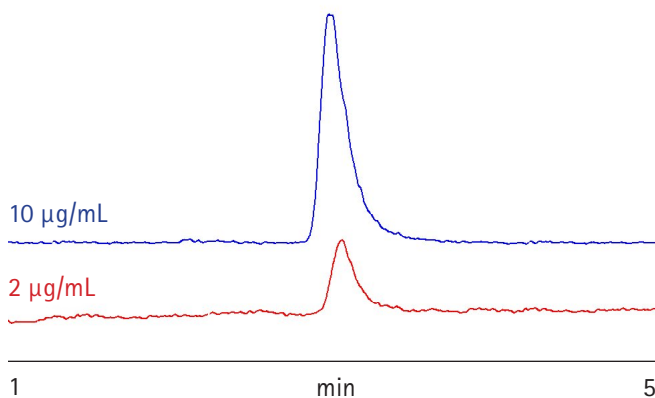

**Figure 1.** Detection of two concentrations of fentanyl within the range 0.5–200 µg/mL.

The peak area measured for every concentration was used to generate a calibration curve as shown in Figure 2 that indicates good linearity over a wide concentration range. The limit of detection was determined at the 1 µg fentanyl/mL loading as this resulted in a peak signal to noise ratio of 3.4; this LOD represents 10 ng on-column loading.

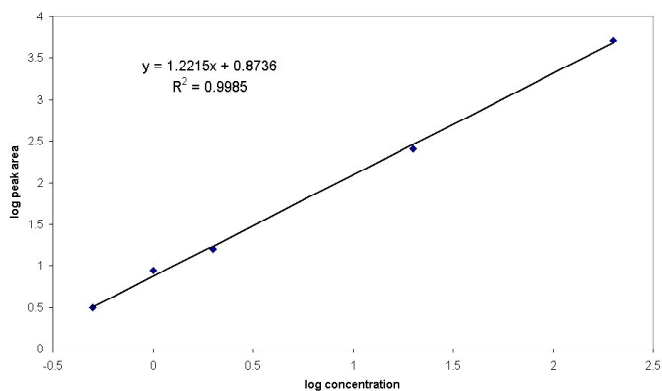

**Figure 1.** Calibration curve for fentanyl (log-log plot).

## Conclusion

Varian ELSD successfully revealed an LOD for fentanyl at 10 ng on column. The Varian ELS detector surpasses other ELSDs for low temperature HPLC applications with semi-volatile compounds. Its innovative design represents the next generation of ELSD technology, providing optimum performance across a diverse range of HPLC applications. The Varian ELS detector's unique gas control permits evaporation of high boiling solvents at very low temperatures. For example, 100 % water at a flow rate of 5 mL/min can be removed at 30 °C. The novel design of the Varian ELS detector provides superior performance compared to detectors from other vendors for the analysis of semi-volatile compounds.

For Forensic Use only.  
Information is subject to change without notice.

---

*These data represent typical results. For further information, contact your local Varian Sales Office.*

Polymer Laboratories, the PL Logo, Varian and the Varian Logo are trademarks or registered trademarks of Varian, Inc. in the U.S. and other countries.  
© 2008 Varian, Inc.



**Polymer Laboratories**

Now a part of Varian, Inc.

Varian, Inc.

[www.varianinc.com](http://www.varianinc.com)

North America: 800.926.3000 – 925.939.2400

Europe: *The Netherlands*: 31.118.67.1000

Asia Pacific: *Australia*: 613.9560.7133

Latin America: *Brazil*: 55.11.3238.0400



**VARIAN**