

## 17 Minute D2712 Analysis of Impurities in Propylene Using PLOT Columns


Propylene production exceeds that of most other hydrocarbons worldwide, as it is a key component in many hard plastics, primarily polypropylene, that are used in a broad spectrum of industries. Propylene can be generated by several methods, which utilize various catalysts to increase production efficiency. Methods include recovering propylene as a byproduct from the steam cracking of liquid feedstocks for ethylene production (e.g. naphtha), from the off-gases produced in fluid catalytic cracking units in refineries, or through direct methods, such as propane dehydration. Regardless of the production method, high purity product is extremely important to prevent damage to the catalysts used in production.

Purity often is determined using ASTM Method D2712, a gas chromatography method for determining part-per-million levels of hydrocarbon impurities in propylene concentrates. This test can be performed on any gas chromatographic system capable of detecting compounds at concentrations of at least 20ppm. While a wide variety of column choices are allowed by the method, the packed columns that are commonly used generally involve complex, multiple column setups, and often suffer from poorly resolved peaks or long run times.

Capillary PLOT columns can be an effective alternative to packed columns for propylene analysis; alumina PLOT columns, in particular, offer a high degree of selectivity for resolving low molecular weight hydrocarbons. Deactivation type can also enhance the separation between difficult to resolve compounds. Here, an Rt®-Alumina BOND column with a Na<sub>2</sub>SO<sub>4</sub> deactivation was used to illustrate a simple single column setup that results in fast, baseline resolution of low molecular weight hydrocarbons from propylene.

Separation of the compounds typically encountered in a propylene stream is often difficult to achieve using packed columns. In contrast, all compounds are fully resolved on an Rt®-Alumina BOND/Na<sub>2</sub>SO<sub>4</sub> PLOT column. These highly efficient columns provide excellent separation, even for difficult to resolve compounds like cyclopropane and propylene. The Rt®-Alumina BOND/Na<sub>2</sub>SO<sub>4</sub> PLOT column also exhibits high capacity or loadability, as evidenced by the minimal amount of tailing on the propylene

**Figure 1** Rt®-Alumina BOND columns provide fast, complete separation of hydrocarbon impurities in propylene.

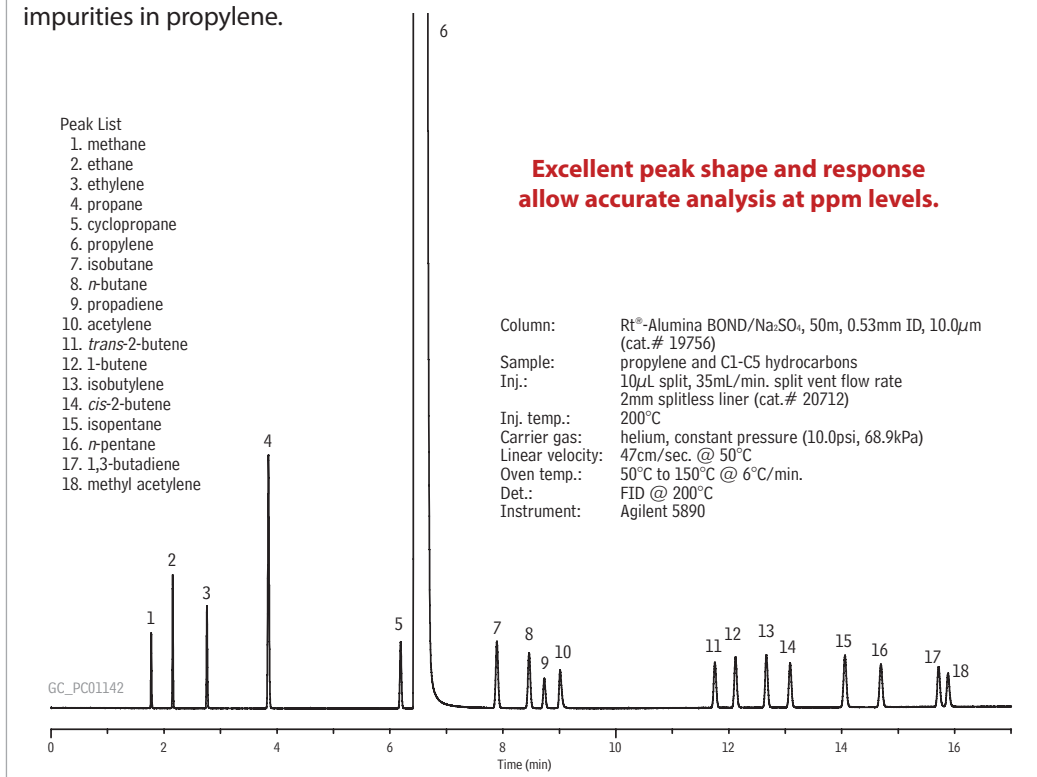

peak. Improved peak shape for high concentration compounds minimizes the difficulty in identifying and quantifying other compounds that elute near the tailing edge of the major peak.

In addition to the complete separation of all compounds on a single column, another advantage of using the Rt®-Alumina BOND/Na<sub>2</sub>SO<sub>4</sub> PLOT column is the fast analysis time than can be achieved. In comparison to packed column methods, which can require multiple columns and up to 45 minutes per run, the total run time using the Rt®-Alumina BOND/Na<sub>2</sub>SO<sub>4</sub> PLOT column is only 17 minutes. High sample throughput is further supported by the short temperature program used here, as compared to some of the isothermal conditions and longer run times noted in the method.

In conclusion, the analysis of impurities in propylene can be significantly improved by using a single Rt®-Alumina BOND/Na<sub>2</sub>SO<sub>4</sub> PLOT column instead of a multiple-column packed column setup. When testing for hydrocarbon impurities in propylene using ASTM D2712-91, the use of an Rt®-Alumina BOND/Na<sub>2</sub>SO<sub>4</sub> column provides the greatest degree of separation in the least amount of time.

### Rt®-Alumina BOND/Na<sub>2</sub>SO<sub>4</sub> Columns (fused silica PLOT) (Na<sub>2</sub>SO<sub>4</sub> deactivation)

Rt®-Alumina BOND/Na<sub>2</sub>SO<sub>4</sub> columns replace GS-Alumina, CP-Al<sub>2</sub>O<sub>3</sub>/Na<sub>2</sub>SO<sub>4</sub>, HP-PLOT S, and AT Alumina columns. Switch today and benefit from:

- More symmetric peaks, due to higher loadability.
- High response for low-level impurities.
- Predictable retention times run-to-run and column-to-column.
- No particle loss, due to unique bonding technology.

ID	df (μm)	temp. limits	length	cat. #
0.32mm	5	to 200°C	30-Meter	19757
0.32mm	5	to 200°C	50-Meter	19758
0.53mm	10	to 200°C	30-Meter	19755
0.53mm	10	to 200°C	50-Meter	19756

**RESTEK**  **REFINED**  
innovative petrochemical solutions  
Columns, standards, and industry experts. Visit:  
[www.restek.com/petro](http://www.restek.com/petro)

### Questions?

Contact [support@restek.com](mailto:support@restek.com) for helpful, knowledgeable technical support.

#### PATENTS & TRADEMARKS

Restek® patents and trademarks are the property of Restek Corporation. (See [www.restek.com/Patents-Trademarks](http://www.restek.com/Patents-Trademarks) for full list.) Other trademarks appearing in Restek® literature or on its website are the property of their respective owners. The Restek® registered trademarks used here are registered in the United States and may also be registered in other countries.

### Restek Electronic Leak Detector

*Why have a small leak turn into a costly repair? Protect your data and analytical column by using a Restek Leak Detector.*

Features & Benefits include:

- Optimized sample flow path.
- New ergonomic, hand-held design.
- Rugged side grips for added durability.
- Handy probe storage for cleanliness and convenience.
- Longer lasting battery, up to 6 hours of continuous use.
- Automatic shut-off.
- A convenient carrying and storage case.
- Easy to clean probe assembly.
- A universal charger set (US, European, UK, and Australian plugs included).



Backed by a 1-year warranty, the new Restek Leak Detector sets an industry standard for performance and affordability in hand-held leak detectors.

#### Leak Detector Facts

Detectable gases: helium, nitrogen, argon, carbon dioxide, hydrogen

Battery: Rechargeable Ni-MH  
internal battery pack  
(6 hours normal operation)

Operating Temp. Range: 32°-120°F (0°-48°C)  
Humidity Range: 0-97%  
Warranty: one year  
Certifications: CE, Ex, Japan  
Compliance: WEEE, RoHS

Gas	Minimum Detectable Leak Rate (atm cc/sec.)	Indicating LED Light Color
Helium	1.0 x 10 <sup>5</sup>	red
Hydrogen*	1.0 x 10 <sup>5</sup>	red
Nitrogen	1.4 x 10 <sup>3</sup>	yellow
Argon	1.0 x 10 <sup>4</sup>	yellow
Carbon Dioxide	1.0 x 10 <sup>4</sup>	yellow

Description	qty.	cat.#
Leak Detector with Hard-Sided Carrying Case and Universal Charger Set (US, UK, European, Australian)	ea.	22839
Soft-Side Storage Case	ea.	22657
Small Probe Adaptor	ea.	22658

Avoid using liquid leak detectors on a GC! Liquids can be drawn into the system.

\*Caution: The Restek Electronic Leak Detector is designed to detect trace amounts of hydrogen in a noncombustible environment. It is NOT designed for determining leaks in a combustible environment. A combustible gas detector should be used for determining combustible gas leaks under any condition. The Restek Electronic Leak Detector may be used for determining trace amounts of hydrogen in a GC environment only.

**RESTEK**

Lit. Cat.# PCAN1202  
© 2009 Restek Corporation. All rights reserved.  
Printed in the U.S.A.

U.S. • 110 Benner Circle • Bellefonte, PA 16823 • 1-814-353-1300 • 1-800-356-1688 • fax: 1-814-353-1309 • [www.restek.com](http://www.restek.com)  
China • phone: +86-10-5629-6620 • fax: +86-10-5814-3980 • [cn.restek.com](http://cn.restek.com)  
France • phone: +33 (0)1 60 78 32 10 • fax: +33 (0)1 60 78 70 90 • [www.restek.fr](http://www.restek.fr)  
Germany • phone: +49 (0)6172 2797 0 • fax: +49 (0)6172 2797 77 • [www.restekgmbh.de](http://www.restekgmbh.de)  
Italy • phone: +39-02-7610037 • fax: +39-02-70100100 • [www.superchrom.it](http://www.superchrom.it)  
Japan • phone: +81 (3)6459 0025 • fax: +81 (3)6459 0025 • e-mail: [restekjapan@restek.com](mailto:restekjapan@restek.com)  
UK • phone: +44 (0)1494 563377 • fax: +44 (0)1494 564990 • [www.thamesrestek.co.uk](http://www.thamesrestek.co.uk)

